

High-Precision 5DoF Tracking and Visualization of Catheter Placement in External Ventricular Drainage of the Brain using Augmented Reality

XUETONG SUN, University of Maryland College Park, USA

SARAH MURTHI, University of Maryland School of Medicine, USA

GARY SCHWARTZBAUER, University of Maryland School of Medicine, USA

AMITABH VARSHNEY, University of Maryland College Park, USA

External ventricular drainage (EVD) is a high-risk medical procedure that involves inserting a catheter inside a patient's skull, through the brain and into a ventricle, to drain cerebrospinal fluid relieving elevated intracranial pressure. Once the catheter has entered the skull its tip cannot be seen. The neurosurgeon has to imagine its location inside the cranium and direct it towards the ventricle using only anatomic landmarks. The EVD catheter is thin and thus hard to track using infra-red depth sensors. Traditional optical tracking using fiducial or other markers inevitably changes the shape or weight of the medical instrument. We present an augmented reality (AR) system that depicts the catheter for EVD and a new technique to precisely track the catheter inside the skull. Our technique uses a new linear marker detection method that requires minimal changes to the catheter and is well-suited for tracking other thin medical devices that require high-precision tracking.

CCS Concepts: • **Computing methodologies** → **Tracking; Mixed / augmented reality.**

Additional Key Words and Phrases: Augmented reality, 5DoF tracking, external ventricular drain, assisted surgery, catheter placement

ACM Reference Format:

Xuetong Sun, Sarah Murthi, Gary Schwartzbauer, and Amitabh Varshney. 2019. High-Precision 5DoF Tracking and Visualization of Catheter Placement in External Ventricular Drainage of the Brain using Augmented Reality. *ACM Trans. Comput. Healthcare* 1, 1, Article 1 (January 2019), 19 pages. <https://doi.org/10.1145/3365678>

1 INTRODUCTION

External ventricular drain (EVD) placement involves inserting a very small clear plastic tube into a lateral ventricle of the brain. Once the catheter is inside the skull, its position can no longer be directly observed, and the neurosurgeon must rely on his or her experience and knowledge of human anatomy to guide placement of the catheter. Huyette *et al.* [2008] and Kakarla *et al.* [2008] retrospectively assess the accuracy of ventriculostomy catheter placement by comparing postprocedure CT scans with preoperative scans. The former study includes 98 ventriculostomy catheter placements and finds that in the author's institution, it requires on average 2 passes to successfully place the catheter, and 22.4% of those successful placements end up in nonventricular spaces. The

Authors' addresses: Xuetong Sun, University of Maryland College Park, 8125 Paint Branch Drive, College Park, MD, 20740, USA, xtsun@umiacs.umd.edu; Sarah Murthi, University of Maryland School of Medicine, 901 Hillstead Drive, Lutherville, MD, 21096, USA, smurthi@umm.edu; Gary Schwartzbauer, University of Maryland School of Medicine, University of Maryland Medical Center Department of Neurosurgery, Suite 12D, Baltimore, MD, 21201, USA, GSchwartzbauer@som.umaryland.edu; Amitabh Varshney, University of Maryland College Park, College Park, MD, USA, varshney@umiacs.umd.edu.

Permission to make digital or hard copies of all or part of this work for personal or classroom use is granted without fee provided that copies are not made or distributed for profit or commercial advantage and that copies bear this notice and the full citation on the first page. Copyrights for components of this work owned by others than ACM must be honored. Abstracting with credit is permitted. To copy otherwise, or republish, to post on servers or to redistribute to lists, requires prior specific permission and/or a fee. Request permissions from permissions@acm.org.

© 2019 Association for Computing Machinery.

2637-8051/2019/1-ART1 \$15.00

<https://doi.org/10.1145/3365678>

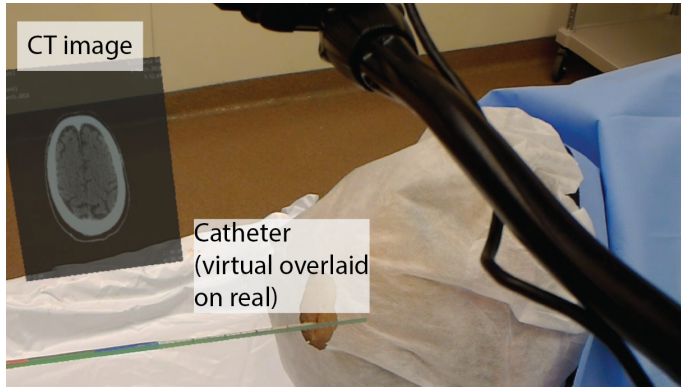


Fig. 1. This figure shows our results in a realistic surgical scenario where EVD is performed on a cadaveric head. The image shown above has been acquired on a Microsoft HoloLens with its mixed reality capture functionality and depicts what a surgeon using our system sees. Additional information could be shown such as the CT slice at the tip of the catheter if a CT volume is registered to the patient. The CT image shown in this figure serves as an illustration of this potential.

latter includes studies of 346 patients and finds that 13% of the catheter placements are suboptimal, resulting sometimes in unfunctional drainage. Furthermore, Woo *et al.* [2019] find that catheter misplacement is a significant independent predictor of catheter-associated hemorrhage. In a radiographic simulation, Robertson *et al.* [2017] find that the traditional method of EVD trajectory selection and placement is predicted to have a 19% chance to impact a cortical vein. These results show that there is still much room for improvement. A method of visualizing the location of the catheter inside the skull would be of great assistance to the surgeon.

A few EVD visualization techniques have been proposed. Cutler *et al.* [2017] have developed a system in which an optical marker is attached to the catheter and tracked by the camera on a head-mounted display (HMD). Other medical instrument tracking techniques by Wany *et al.* [2010], Najafi *et al.* [2015; 2011], Stolka *et al.* [2014] and Fan *et al.* [2017] make use of markers of different kinds.

Microsoft Kinect has been successfully used to reconstruct 3D meshes representing humans at real-time rates [Du *et al.* 2019]. However, our preliminary tests with Microsoft Kinect 2.0 showed that the thinness of the catheter makes it hard to detect and track with commodity depth sensors. The shortcomings of infrared depth sensing, in this case, are out of the scope of this paper¹. Instead, we devise a new optical marker and tracking technique, suitable for augmented reality. We label a portion of the catheter with three distinct colors. One design principle we have observed after consulting our medical collaborators is making minimal changes to the catheter. Our modification does not change the catheter in any way that would make it feel different to operate. We develop an algorithm to detect the color bands and then use them to calculate the position of the catheter. This way, even if the tip of the needle is occluded, we still know where it is and are able to visualize it, as long as enough of the colored portion remains visible. We display a virtual catheter overlaid on the real catheter directly in the user's field of view using a see-through Microsoft HoloLens, which allows the surgeon to better focus on the patient while still having access to the relevant data and provides better depth perception and understanding of the operating context. We only need to do a one-time calibration to determine the relation between the HoloLens and the camera.

¹See supplementary video for a demonstration of how commodity depth sensors are unsuitable for catheter tracking

Testing shows our system achieves high accuracy and low latency. We also show the usefulness of our system in a realistic surgical environment on a cadaveric head. An example of the view directly observed by the surgeon is shown in Fig. 1.

Our system takes a step beyond Cutler *et al.*'s pioneering research [Cutler *et al.* 2017] and improves on several aspects. First, our tracking technique does not require significant changes to the shape and weight of the catheter. Second, since we use a stationary camera for tracking, it does not require the user of the head-mounted display to be looking at the catheter to track. This allows the surgeon to freely look anywhere without losing the tracking of the catheter. Finally, the capability of our system is not tied to the HMD. We empirically observed a lag of 1.43s in Cutler *et al.* [2017]'s video demonstration², which is likely caused by the HMD's inability to keep up with the processing. In our system, the images from the camera, as well as the medical volume are processed separately on another machine, and results are sent to the HMD wirelessly. This allows for faster and more accurate sensing and higher fidelity medical images. Our system can be naturally integrated with existing medical image registration techniques. A proposed example is illustrated in 1 where the CT slice at the tip of the catheter is displayed if the CT volume is registered with the patient. Due to the scope of this study, we do not perform the medical image registration but refer interested readers to surveys by Kersten-Oertel *et al.* [2013] and Meola *et al.* [2016].

In short, we built an augmented reality EVD tracking and visualization system that

- overlays a virtual catheter onto a user's field-of-view, mimicking the position of the real catheter,
- leaves the catheter functionally unchanged, and
- is accurate and responsive.

The remainder of this paper is organized as follows. In Section 2, we cover past research on enhancing surgeon performance in EVD procedures, as well as cases in which AR is used in neurosurgery. In Section 3, we give an overview of our system and introduce how we visualize the catheter based on the result from our algorithm. We cover in detail our algorithm to calculate the position of the catheter in Section 4. In section 5, we show the stability, accuracy, and latency of our system. Finally, in Section 6, we discuss some limitations of our system, initial response from medical professionals, and future work.

2 RELATED WORK

External ventricular drainage has undergone numerous iterations in materials and techniques since it was first performed in the 1740s. The complete documentation of the evolution of EVD is out of scope for this paper; readers can refer to Srinivasan *et al.* [2014]. In this section, we will review recent developments in EVD catheter placement techniques. In addition, we discuss augmented reality use cases in neurosurgery.

2.1 Catheter Placement

Proper catheter placement is key to the success of an EVD procedure. A 2016 Neurocritical Care Society study (Fried *et al.* [2016]) found that with a stabilization tripod ("Ghajar guide") or other technical adjuncts such as CT guidance, stereotactic navigation could improve accuracy and/or lower the number of EVD procedures performed on a patient.

The "Ghajar guide" is a catheterization assistance device in current clinical use, invented by Jamshid Ghajar in 1985. It is a tripod-shaped device that can be securely placed on the patient's skull; the catheter travels along the axis of the device and can be stabilized as it goes into the skull.

²We observed this at 50s and 51s in video <https://youtu.be/qyqkWW9f41Q>

A study by O’Leary *et al.* [2000] found that successful catheterization can be achieved either using a Ghajar guide or freehand, but that a smaller distance to target was achieved with the Ghajar guide.

For ventricle exploration and catheter placement training, Phillips and John [2000] developed a simple web application that lets trainee surgeons practice simulated catheterization (catheter placement) via a personal computer. Cros *et al.* [2002] incorporated haptic feedback into the ventriculostomy simulator; users feel a “pop” sensation when the catheter pierces the ventricular surface.

Krombach *et al.* [2000] conducted free-hand catheterization simulations before performing the actual surgery. In simulations, MRI images were registered onto the patient’s head with fiducials. A pointer instrument was tracked by infrared diodes attached to it. The surgeons used the pointer to virtually move the catheter and the position of the catheter was evaluated.

Luciano *et al.* [2005] developed the *ImmersiveTouch* ventriculostomy simulation system. Stereoscopic goggles are tracked electromagnetically and represent the head position. A hand stylus is tracked mechanically and can offer different resistance sensations to simulate catheter moving in different types of tissue. This way, the displayed content can change according to the user’s point of view and the virtual catheter is visualized based on the location of the hand stylus. Haptic feedback is provided to perceive the interaction between the virtual catheter and the virtual brain model. *ImmersiveTouch* is used in studies by Banerjee *et al.* [2007], Lemole *et al.* [2007], Schirmer *et al.* [2013] and Yudkowsky *et al.* [2013].

Tai *et al.* [2015] 3D-printed an actual physical phantom head (manikin head for medical procedure simulations) from the reconstruction of CT images and used the brain model as an EVD training platform. This platform provides a realistic anatomical structure and visual/haptic feedback.

The most recent experimental EVD development is by Li *et al.* [2018] where the neurosurgeon guides the catheter by aligning it to the displayed trajectory which is shown in an HMD. In an effort to track the catheter, Cutler *et al.* [2017] attach an optical marker, in this case, a piece of paper, to a rigid catheter. The marker’s, and therefore the catheter’s position is tracked by the camera on an HMD, which displays the virtual catheter image as well as a 3D model of the damaged part of the brain. This way, as long as the marker is in the camera’s field of view, the catheter can be visually tracked, even when the tip is occluded. The system compellingly demonstrates how the advances in sensing and displays can create intuitive and reliable assistance to neurosurgery. Somewhat similar to Cutler *et al.* [2017] but used in biopsy and ablation are Lin *et al.*’s *HoloNeedle* [Lin *et al.* 2018] and Kuzhagaliyev *et al.* [2018], where the needle is tracked using the *OptiTrack*³ system and a virtual needle is displayed in an AR headset to align with the real one. In Lin *et al.*’s *HoloNeedle*, the biopsy needle’s shape is further obtained with embedded Fiber Bragg Grating sensors to take the needle bending into consideration. All the systems mentioned above make a significant change to the shapes of the instruments to accommodate their tracking techniques which our method avoids (more detail in Section 4). Najafi *et al.* [2015; 2011] use a closed-form formula to calculate the trajectory of a needle instrument based on the live footage from a single camera attached to an ultrasound probe and guide the needle angle to reach the target shown in the ultrasound image. Our system is different in that the exact location of the catheter tip is calculated visualized directly in the user’s field of view via an AR HMD. Stolka *et al.* [2014] use stereo cameras to detect the 5DOF information of a needle marked with pseudo random binary sequence (PRBS) patterns and display the needle in the ultrasound image or project a line on the patient’s skin to mimic the needle’s location. A generalized version incorporating multiple medical imaging and probing modalities has been proposed in Basafa *et al.* [2017]. Our system is different in that it uses

³<https://optitrack.com/>

perspective foreshortening of color bands on the catheter to estimate the tip location from a single camera with higher precision than the prior art.

2.2 Augmented Reality Interventions for Neurosurgery

One type of augmented reality technique being used in neurosurgery is overlaying detailed preoperative medical image on intraoperative images. Masutani *et al.* [1998] experimented with overlaying preoperative 3D vascular models onto intraoperative X-ray fluoroscopy images via medical fiducial markers. Two clinical test cases showed the registration reprojection displacement to be below 2.6 mm. Lovo *et al.* [2007] reconstructed volumes from cerebral MR scans and overlaid the volumes onto intraoperative cerebral images.

One step further is to track the imaging probe (or microscope) during surgery and overlay meaningful information such as anatomy models onto the intraoperative images. Edwards *et al.* [1995; 2004; 2000] developed and tested an AR microscope-assisted guided intervention system that tracked the microscope and overlaid 3D medical images on the two eyepieces. Shahidi *et al.* [1998], Scholz *et al.* [1998] experimented with similar setups using surgical endoscopes. Kockro *et al.* [2009] developed a hand-held AR system, *Dex-Ray*, that overlays medical volumes or other images onto a live stream video. Low *et al.* [2010] used *Dex-Ray* integrated with the *Dextroscope* system (an immersive medical image viewing system) and performed meningioma (a type of usually noncancerous brain tumor) excision on five patients. Inoue *et al.* [2013] tracked off-the-shelf webcams to overlay anatomical medical structures on the webcam images.

Sauer *et al.* [2001] and Maurer *et al.* [2001] developed an AR video see-through surgery navigation HMD and demonstrated its use on a phantom head with encouraging results. Two color cameras record the real-world scene, and one additional camera tracks the retroreflective optical markers attached to the phantom head. A medical MR (magnetic resonance) volume aligned with the head phantom is displayed stereoscopically on the HMD. Abe *et al.* [2013] develop an AR guidance system for percutaneous vertebroplasty where the insertion location and intended insertion orientation is displayed in an AR HMD. Trials on the phantom show improved accuracy using this system, and successful clinical trials demonstrate practical usability. Abhari *et al.* [2014] engineer a mixed reality system that facilitates the training and planning for a brain tumor resection procedure and demonstrated the greatly improved performance of junior residents and the reduction in time to perform clinically relevant tasks by clinicians. Li *et al.* [2018] conduct a clinical EVD trial where manually aligned CT holograms are shown in an AR headset to display the catheter placement trajectory and target location. The catheter is not tracked or visualized, but it took the AR-assisted group fewer passes on average to complete the procedure. The AR-assisted group also had a lower average deviation from the target. Azimi *et al.* [2018] develop a mixed reality surgical training system that integrates functionalities such as preoperative procedure visualization and real-time performance assessment and demonstrate a catheter placement training session where the system informs the trainee of the orientation error, though the system's tracking accuracy is not reported. Very recently, Meola *et al.* [2016] and Guha *et al.* [2017] present two thorough surveys on the past work in which AR is used for neurosurgery.

3 SYSTEM OVERVIEW

Our system consists of three components: a sensing unit, a processing unit and a display unit in addition to the modified catheter itself. The functions of each component are described in Section 3.1, as well as the actual hardware used for each component. The way the system is operated in our experiment is described in Section 3.2. Finally, the calibration between the sensing unit and the display unit is described in detail in Section 3.3.

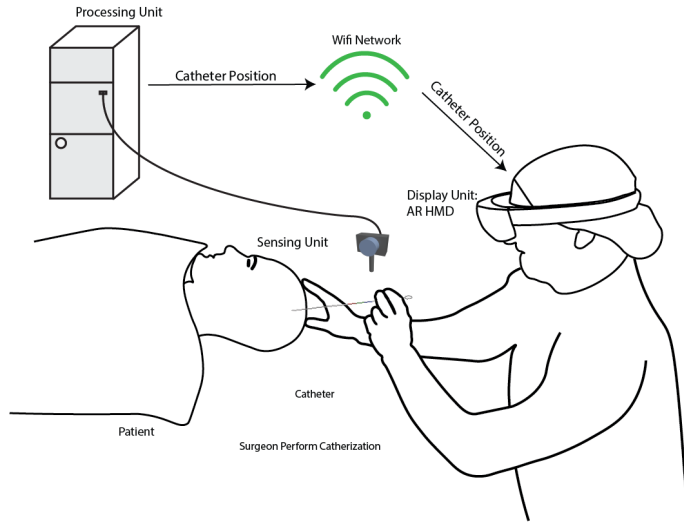


Fig. 2. System Overview

3.1 System Components

The sensing unit captures the live footage of the operation area that contains the modified catheter. The processing unit analyzes the footage and calculates the catheter's position in the camera's reference system (camera space), which is then sent via a wireless network to the display unit. The display unit uses a transformation obtained at the calibration step (more detail in Section 3.3) to transform the received catheter's location into the world reference system (world space) and displays the virtual catheter at that transformed location to overlay the physical catheter. A general illustration of the system, as well as the intended use scenario, can be seen in Fig. 2. The workflow of our system is depicted in Fig. 3. An actual view captured using HoloLens's mixed reality capture function is shown in Fig. 1.

The sensing unit is an off-the-shelf Logitech c920 web camera on a tripod. The reason we use a separate camera, rather than the one integrated into the display, is to avoid being limited by the quality of the integrated camera and the processing capabilities of the display, as well as reduce network latency. The processing unit is an Alienware laptop computer with an Intel i7 7820HK processor running at 2.9GHz. The display unit is a Microsoft HoloLens tetherless AR head-mounted display.

The catheter used in our experiment is a Codman® EDS 3™ clear ventricular CSF catheter. This catheter measures 35 cm in length which is typical of catheters used in EVD. Fried *et al.* [2016] suggest that, in surgical scenarios, the catheter should not penetrate the skull by more than 6.5 cm, therefore we place the color bands 7 cm away from the tip. We use three color bands, each 3.8 cm in length (see Fig. 5 for an illustration).

3.2 System Operation

When using this system, the user wears the HMD which displays a virtual catheter. The virtual catheter can be dragged around in the world space with hand gestures. After the user manually aligns the virtual catheter with the physical one observed through the HMD, the user issues a calibration command which triggers the system to calculate the mapping from the camera space to the world space. The system then uses this mapping to transform the catheter's location in the

camera space into the world space as mentioned above for the subsequent frames, until a new calibration command is issued when the users see fit.

In the experiment, the surgeons held the rear portion of the catheter as illustrated in Fig. 2 to avoid occluding the color bands.

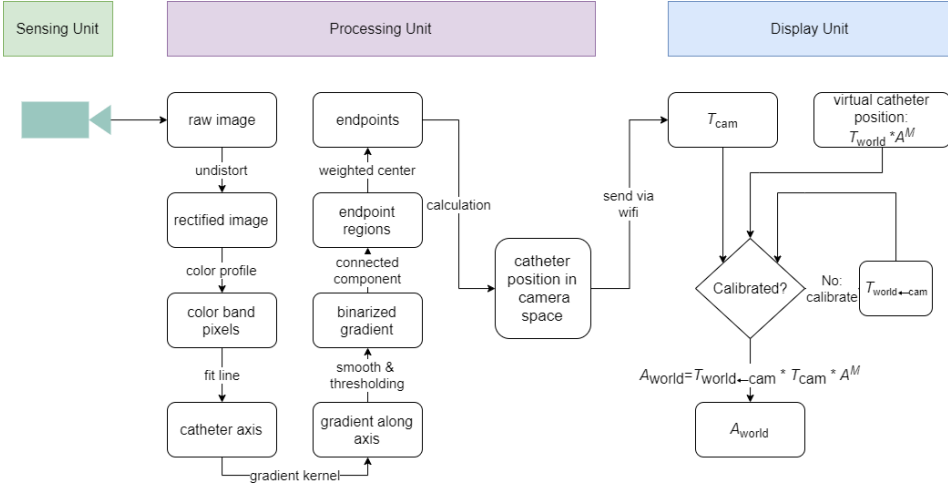


Fig. 3. The workflow of the system

3.3 Reference System mapping

Our algorithm calculates the position of the catheter in the camera space. To be able to visualize the catheter in the HMD, a way to transform from the camera space to the world space is required. We achieve this by doing a one-time calibration with the calculated catheter position in the camera space and the virtual catheter position in the world space. Suppose the coordinate of the catheter in its own reference system (model space) is A^M . At a certain frame, T_{cam} and T_{world} transform A^M into the camera space ($A_{cam} = T_{cam}A^M$) and the world space ($A_{world} = T_{world}A^M$), respectively. We want to find a transformation $T_{world \leftarrow cam}$ that will transform from the camera space to the world space.

$$T_{world \leftarrow cam} T_{cam} A^M = T_{world} A^M \quad (1)$$

In order for this to work with every A^M , we simply take

$$T_{world \leftarrow cam} = T_{world} T_{cam}^{-1} \quad (2)$$

Then with every frame where a new T_{cam} is calculated from the position of the catheter in the image, we can calculate the corresponding T_{world} and display the virtual catheter. Reference system mapping is illustrated in Fig. 4

4 CATHETER TRACKING

We present a novel method of tracking the 3D position of the catheter in real time, enabled by three color bands painted on the catheter. The three color bands are adjacent, and we know each of their lengths and locations relative to the catheter; the colors only need to be sufficiently distinct to be identified in the image (see Fig. 5).

We use a pinhole model to represent the camera. As seen in Fig. 6, P is the center of projection of the pinhole model and is the origin point in camera space. We observe in the image the 2D

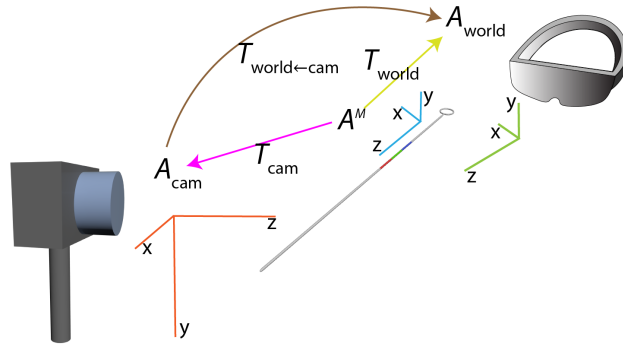


Fig. 4. Reference system mapping

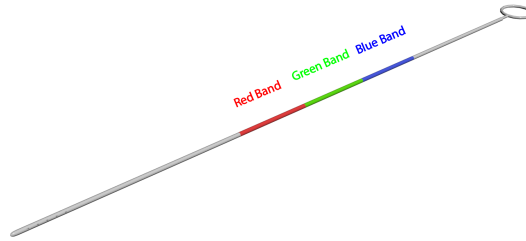


Fig. 5. A drawing of the catheter and the color bands. The color bands need to be distinct and adjacent. The lengths of the three color bands, as well as the uncolored forward portion (from the catheter tip to the beginning of the first color band) of the catheter, are known. With the lengths and the positions of the color band endpoints detected in camera space, we can calculate the 5DOF (no roll) information of the catheter, and infer the position of the tip.

coordinates of the catheter A' , B' , and C' (Fig. 6 shows three endpoints of two color bands as an example). Given that we know the lengths of the color bands $|AB|$ and $|BC|$, this becomes a simplified version of the perspective three-point problem (P3P) thoroughly studied and documented in [Ameller et al. 2000; Gao et al. 2003; Marchand et al. 2016; Quan and Lan 1999]. In a general P3P problem, there could be as many as four solutions. In our case, where the three points are collinear, there could be two solutions, of which only one is desired. Determining the correct solution requires finding the angle between the catheter and its image in the image plane, shown in Fig. 6.

We describe our approach to the P3P problem below. First, we use a geometric method to find α in Section 4.1. Then we calculate the position of the catheter in Section 4.2. Finally, we extract the segments' endpoints A' , B' and C' from the image in Section 4.3.

4.1 Angle α

We denote the three endpoints of two consecutive color bands as A , B , and C in Fig 6, and the center of projection as P . The images of A , B and C are A' , B' and C' on the image plane. Given the camera intrinsics which can be obtained by a one-time calibration, we can explicitly represent P ,

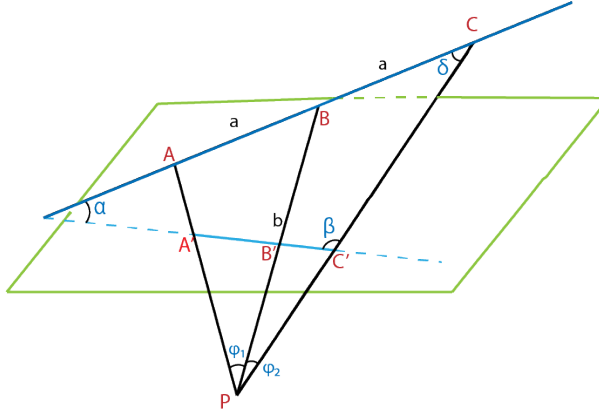


Fig. 6. We need to find the angle α between the catheter and its image. Let A , B , and C be three endpoints of two consecutive color bands. The color bands are of equal length a . P is the center of projection in the pinhole camera model. The distance between B and P is b

A' , B' and C' with exact coordinates in pixels. We can calculate the angles

$$\angle APB = \varphi_1 = \arccos \frac{\mathbf{PA}' \cdot \mathbf{PB}'}{|\mathbf{PA}'| |\mathbf{PB}'|} \quad (3)$$

$$\angle BPC = \varphi_2 = \arccos \frac{\mathbf{PB}' \cdot \mathbf{PC}'}{|\mathbf{PB}'| |\mathbf{PC}'|} \quad (4)$$

Now assume the two color segments are of equal length a (Assume $|AB| = |BC| = a$) and $|PB| = b$. Trigonometric equations give

$$\frac{a}{\sin \varphi_1} = \frac{b}{\sin(\pi - \varphi_1 - \varphi_2 - \delta)} \quad (5)$$

$$\frac{a}{\sin \varphi_2} = \frac{b}{\sin \delta} \quad (6)$$

δ is the angle $\angle ACP$. Solving for δ

$$\delta = \arctan\left(\frac{\sin \varphi_2 \sin(\varphi_1 + \varphi_2)}{(\sin \varphi_1 - \sin \varphi_2 \cos(\varphi_1 + \varphi_2))}\right) \quad (7)$$

Then we can calculate $\alpha = \pi - \beta - \delta$. α could be either positive or negative depending on whether A is farther away from the image plane than C or closer. When A is closer than C (Fig. 6), $\alpha > 0$. When A is farther, $\alpha < 0$.

4.2 Position of Catheter

With the 3D orientation, we can calculate the position of the catheter in camera space. In Fig. 7, AB represents a color band. AT represents the portion of the catheter from the tip to the color band. AT may not be entirely visible from the camera. A' , B' , and T' are the images of A , B and T on the image plane, respectively. We know the lengths of $A'B'$ because we have detected them in the image. We also know the lengths of PA' and PB' as well.

The actual catheter is in the plane formed by P and $T'B'$, and we know its orientation. But it could be on any line that is parallel to TB , for example, $T''B''$. We can set $PA'' = mPA'$. The actual

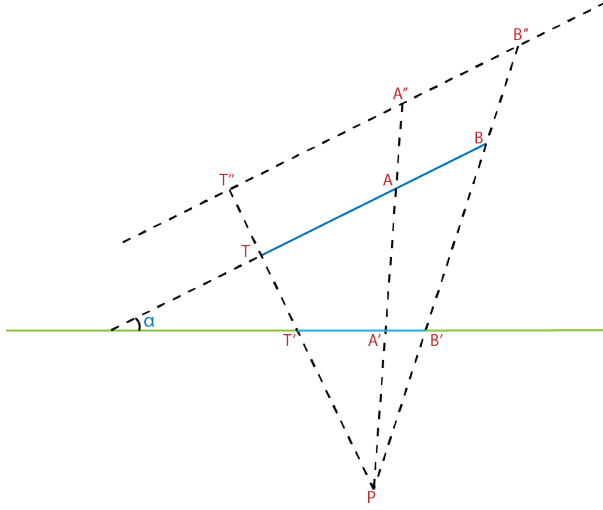


Fig. 7. Finding the position of the catheter in camera space. P is the center of projection. TA is the uncolored forward portion of the catheter. AB is the first color band on the catheter.

ratio m does not really matter because a different ratio only leads to a parallel line to BC . We can assume, for example, $m = 10$, and let $PB'' = kPB'$. Then $A''B'' = PB'' - PA'' = kPB' - PA''$.

We know the angle formed by the catheter and its image α , which is the angle formed by $A''B''$ and $A'B'$.

$$A''B'' \cdot A'B' = |A''B''| |A'B'| \cos \alpha \quad (8)$$

Equation 8 can be further transformed into

$$kPB' \cdot A'B' - PA'' \cdot A'B' = \sqrt{k^2PB'^2 - 2kPB'PA'' + PA''^2} |A'B'| \cos \alpha \quad (9)$$

All the values in Equation 9 are known except for k . We can solve k and thus find the position of B'' . It is worth noting that Equation 9 is a quadratic equation, and there could be two solutions for k . Judging from Fig. 7, if $\alpha > 0$, B should be further away from the image plane than A. Therefore k should be greater than the assumed ratio of $|PA''|$ over $|PA'|$ and vice versa.

Now that we know the length of the catheter color band AB in the real world, we can calculate the position of the color band AB in the camera space.

$$PA = \frac{|AB|}{|A''B''|} PA'' \quad (10)$$

$$PB = \frac{|PA|}{|PA''|} PB'' \quad (11)$$

Since we know where AB is on the catheter, we can calculate the position of the catheter in camera space. For example

$$PT = PA - \frac{|AB|}{|AT|} AB \quad (12)$$

we can calculate the position of the tip in camera space since we know the lengths of the uncolored forward portion of the catheter and the color bands.

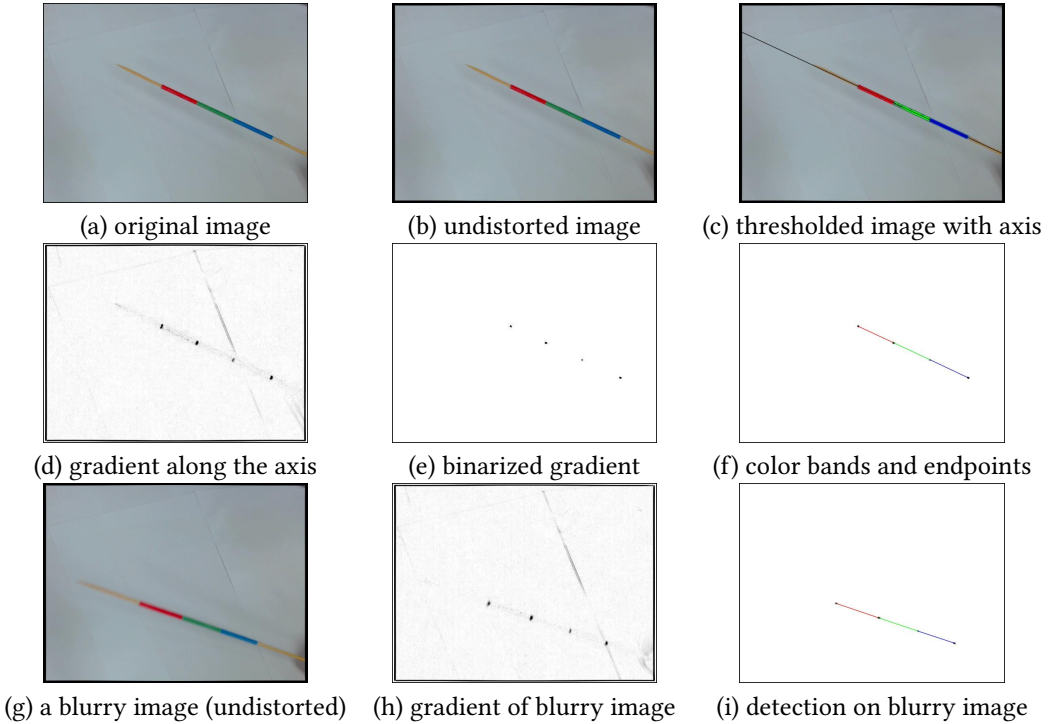


Fig. 8. Detecting endpoints. (g), (h) and (i) show detecting endpoints in an image where the catheter is blurry because of movement. Our algorithm is able to handle this case.

It is worth noting that we can calculate the position of the catheter with two adjacent color bands. We use three color bands to make our system robust against occlusion and improve accuracy when all three are visible.

4.3 Color Band Detection

In the color band detection step, the input is an image I of the catheter (P_{catheter} being all the pixels that belong to the catheter), and the output is the locations of the endpoints of the color bands. The accuracy of the color band detection is the most important factor in finding the catheter tip. To reliably detect the endpoints of the color bands, we develop a new algorithm (see Fig. 3). Starting from the original image (Fig. 8 (a)) and its undistorted result (Fig. 8 (b)), we first use simple thresholds to get the most of the pixels $P_{\text{catheter}}^* \subseteq P_{\text{catheter}}$ of the catheter in the image. We then fit these pixels to a line, which we call the axis L_{axis} of the catheter (Fig. 8 (c)). The gradient $G_{L_{\text{axis}}}$ along the direction of L_{axis} is calculated using a variation of Sobel filter $K_{L_{\text{axis}}}$ that is weighed anisotropically according to L_{axis} (Fig. 8 (d)). $G_{L_{\text{axis}}}$ has high values near the border of two different colors. After smoothing using a median filter, the gradient map is thresholded into binary images $G_{L_{\text{axis}}}^*$ with positive values where the borders are (Fig. 8 (e)). Finally, we take the weighted centers of the connected components of $G_{L_{\text{axis}}}^*$ as the endpoints of color bands (Fig. 8 (f)). Our processing technique is robust against blurry images caused by motion, as seen in Fig. 8 (g, h, i).

5 ACCURACY ANALYSIS

In this section, we analyze the performance of our proposed algorithm. First, we measure the stability of our tracking algorithm. Then we test tracking accuracy on a 2D planar grid as well as a specially designed and 3D-printed grid. Finally, we test the latency compared with a third-party tracker.

5.1 Stability

Given the color segment endpoints detected in the image, our tracking algorithm will output the computed catheter position. The instability in the tracking algorithm comes from random noise in each frame. The noise could cause the same endpoint in two frames to be detected a few pixels apart, even when the catheter stays still.

We measure the stability as the root mean square of the change of calculated tip in camera space in two consecutive frames as in Niehorster *et al.* [2017] while keeping the catheter still. Given n frames, and the tip of the catheter in frame i as \mathbf{x}_i , the stability is measured as

$$S_{RMS} = \sqrt{\frac{1}{n-1} \sum_{i=1}^{n-1} \|\mathbf{x}_i - \mathbf{x}_{i+1}\|^2} \quad (13)$$

Several factors could influence the stability of the tracking algorithm, including lighting condition, thresholds for color segmentation, and distance from the camera to the catheter. In a typical lab setting, our algorithm achieves a stability of 0.33 mm as measured over 870 frames.

5.2 Accuracy over a 2D Grid

To test the accuracy of the tracking algorithm, we move and point the tip of the catheter at the intersections of a grid. The grid, 8.16 cm \times 8.16 cm in size, is printed on a white sheet. This provides enough space to test the accuracy of catheter movement, more than the 6.5 cm suggested by Fried *et al.* [2016]. The setup for this test can be seen in Fig. 9 (a).

We assume the center intersection of the grid to be a reference point. Before the test, a 2D marker is placed on the workbench, and its up and right directions (parallel to the edges of the paper sheet the marker is printed on) in the camera space are detected. The sheet with the grid is then placed on top of the marker with the edges aligned. Therefore, the grid has the same up and right direction as the marker, and with its size known, we know the position of each grid intersection relative to the reference point. When moving along the grid, the catheter's orientation is kept relatively fixed and its tip position in the camera space is recorded. Then the tip positions relative to that when the tip is pointed at the reference point is compared to positions of the grid intersections relative to the reference point.

Fig. 10 shows the catheter tip locations on the grid with the reference point as the origin. Blue circles indicate the grid intersections, and the orange crosses are the detected catheter tips. The average distance from the catheter tip to the corresponding grid intersections is 0.58 mm.

5.3 Accuracy over a 3D Grid

We also demonstrate the accuracy of our algorithm when the catheter is moving in vertical space. To construct a reliable ground truth, we use a 3D-printed structure where square grids of blind holes are on its three faces (see Fig. 9). The centers of the blind holes are $d = 10$ mm apart in both directions which we manually verified with a caliper. Each blind hole is designed to be a cone with 1 mm radius and 3 mm height. On each face, there are 8×8 blind holes.

When testing on each face, one of the center blind holes (for example (m, n) on the 8×8 grid) is chosen as the reference point. The location of the tip when the needle tip is inserted into each

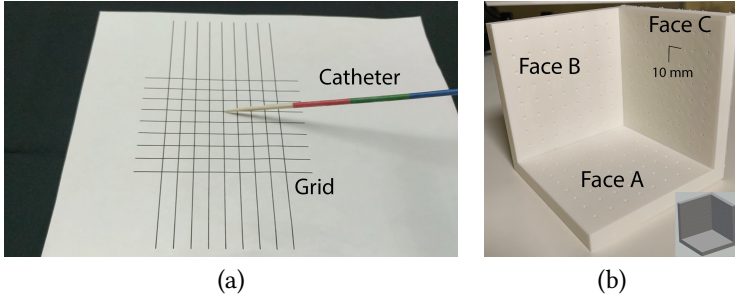


Fig. 9. Setup for testing (a) the tracking accuracy over a 2D grid, and (b) tracking accuracy over a 3D grid with the 3D CAD model in the lower right

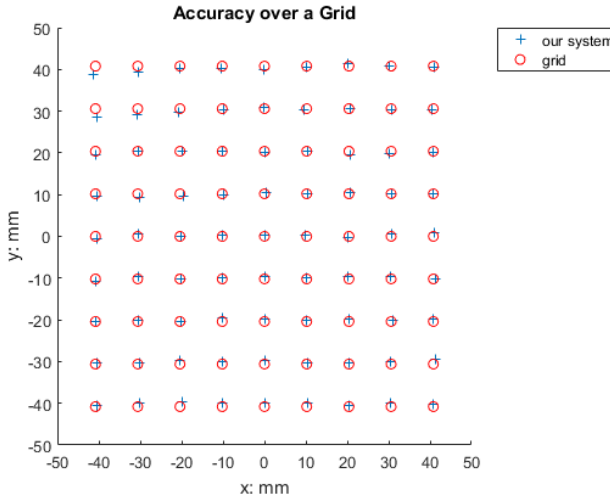


Fig. 10. The accuracy of our catheter tracking approach over the 2D grid. The red circles indicate the grid intersection. The blue crosses indicate the computed catheter tip position.

blind hole (i, j) is recorded as $T(i, j)$. We construct the ground truth $G(i, j)$ as the designed distance of each blind hole to the reference point $G(i, j) = \sqrt{(m - i)^2 + (n - j)^2}d$. The distance between the calculated tip and the reference at each blind hole is $D(i, j) = \|T(i, j) - T(m, n)\|_2$. The average accuracy on the face f is then $Acc_f = \frac{1}{64} \sum_{i,j} |G(i, j) - D(i, j)|$.

In this test, $Acc_A = 0.49$ mm, $Acc_B = 0.93$ mm, $Acc_C = 1.12$ mm. The overall average accuracy on all three faces is 0.85 mm.

5.4 Latency

We measure our tracking system's latency using an HTC Vive tracker which according to [Niehorster et al. 2017] itself has a 22 ms latency. This latency is measured as the time elapsed between the tracker update and our system catheter's location update. In our test, we rapidly move the catheter, which is attached to the tracker, and record for each frame the distance from the catheter tip (tracked with our system and by the HTC Vive tracker) to their original location recorded at the beginning of the test. The distances are then plotted and we manually measure average time by

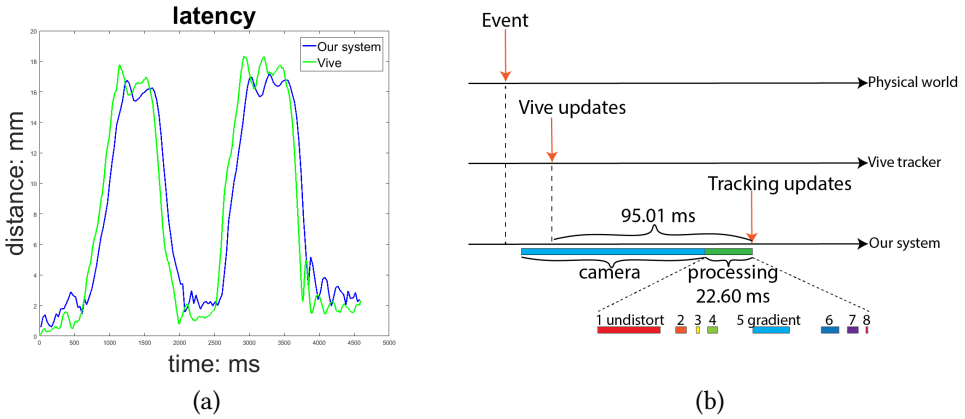


Fig. 11. The latency of our system compared to an HTC Vive tracker (a) and the various components of our system's latency in image capture and processing (b).

ID	Function	Avg time per frame (ms)	Percentage in processing (%)
1	Undistort	10.04	44.42
2	Color segmentation	1.05	4.64
3	Erosion	0.23	1.02
4	Get axis	0.93	4.13
5	Gradient	6.81	30.12
6	Connected components	1.15	5.08
7	Weighted centroids	0.92	4.09
8	Calculate catheter position	0.21	0.92
	Other	1.26	5.58
	Total	22.60	100.00

Table 1. Time breakdown of functions in tracking

which our system lags the tracker. Fig. 11 (a) shows the plotted distances that we recorded. Manual measurements show an average latency of 95.01 ms. A break down of the latency can be seen in Fig. 11 (b).

There are two factors in the latency with respect to the HTC Vive tracker. It takes about 72 ms for our camera (together with the driver, and OpenCV functions) to capture and store the image. The processing takes an additional 22.60 ms on our machine, which uses an Intel i7 7820HK processor running at 2.9GHz. As we show in Table 1, undistorting takes the longest time, 10.05 ms per frame (44.42% of the total processing time). Speed up may be achieved by performing color segmentation first and undistorting only the pixels of the color bands. The next most time-consuming task is calculating the gradient along the catheter axis, (6.81 ms per frame, 30.12% of total processing time). Our current implementation is on the CPU. A GPU is likely to reduce the processing time through parallelization. A professional-grade camera with a low image capture time can greatly reduce the latency.

6 DISCUSSION AND FUTURE WORK

We have demonstrated a novel method of tracking a catheter and projecting it onto an augmented reality display. Better visualization during EVD placement has the potential to make a risky procedure safer and save lives. In combination with CT scan projection of the skull, this could potentially provide the neurosurgeons with a clear view of where the catheter is relative to the insertion target inside the skull of a patient. We address the challenges of significantly enhancing the accuracy and latency of our system over the state-of-the-art augmented reality systems for this procedure such as Cutler *et al.* [2017].

External ventricular drainage is a technically difficult procedure. It involves placing a catheter several centimeters into the brain through tissues of varying density including bone, dura, brain and cerebral spinal fluid. In addition, it is generally performed in bright light with blue sterile drapes. These realities can potentially affect the accuracy of AR tip projection in difficult-to-predict ways and needed to be validated in our study. Furthermore, the AR system should not interfere with procedure performance by not hindering the surgeon placing the drain. A purely computational evaluation of our approach would not have been sufficient to assess the efficacy of our augmented-reality approach in such challenging environments.

In order to validate the true feasibility of AR-assisted EVD placement, we have carried out our evaluation in a realistic experimental environment, which included a cadaveric head, using sterile drapes and the existing EVD placement kits, closely mimicking actual EVD placement in a patient. After inserting the catheter tip at the insertion point, the surgeons advanced the catheter in a straight line. During the process, the displayed virtual catheter projection aligned well with the visible portion of the real catheter and the pace at which the real and the virtual catheter moved matched. The surgeons have reported that the handling of our slightly modified catheter feels identical to a traditional catheter. The surgeons, while aware of the HMD, did not find it cumbersome.

Tests show that our tracking method is accurate with sub-millimeter accuracy and low latency. If further improvements in accuracy and latency were needed, we could do so with the following enhancements. First, a professional-grade camera with a higher resolution, higher dynamic range, and lower latency could improve tracking by enhancing our ability to discern the segment endpoints and reduce the overall latency. With a higher resolution, the camera could be farther away from the catheter without compromising tracking quality, thus allowing a larger tracking area. All this comes with a higher computational burden. At the moment, our algorithm is implemented on a CPU but is highly parallelizable. Implementing a parallel GPU version of the algorithm is a high priority in our future work. At present, we observe around 167 ms end-to-end latency between moving the real catheter and its updating the virtual catheter in the HMD. In our current system, we use an independent camera and a laptop for processing, but it would be desirable to explore an all-in-one setup. This is highly likely with further advances in commodity HMDs. Current-generation AR HMDs often suffer from drift in spatial tracking. In our studies, this has ranged from 2.15 mm to 6.35 mm, depending on the amount of user head movement. Complementing the 3D spatial tracking with 2D optical tracking like in Frantz *et al.* [2018] should be able to improve spatial tracking accuracy.

In our system, the calibration between the camera space and the world space is performed manually to make sure the observed virtual catheter aligns with the observed physical catheter. Therefore very little optical misalignment has been observed in our experiment as long as the user does not remove or adjust how the HMD is worn. We believe that this limitation shall be largely addressed by eye-tracking and better optical alignment in the next-generation HMDs. As the next-generation HMDs support a higher resolution and a wider field-of-view, it should be

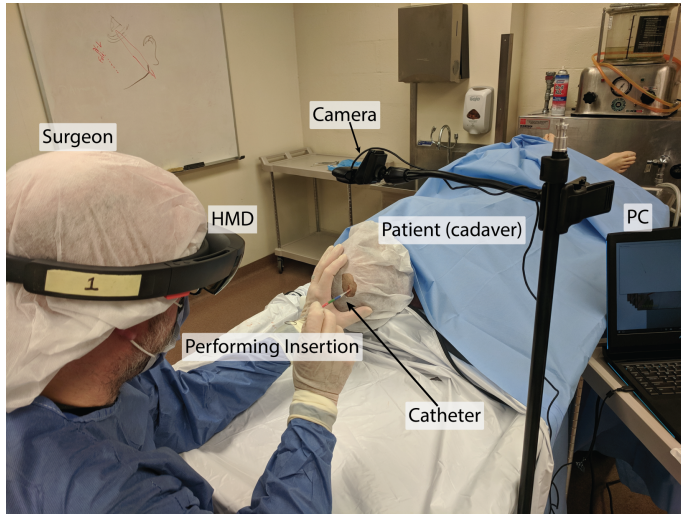


Fig. 12. Our system being used in a cadaver study

possible to further support the presentation of time-critical information to assist in procedures such as EVD. This information could be presented in both the peripheral regions [Sun and Varshney 2018] as well as the foveal regions [Meng et al. 2018] of the surgeon’s field of view.

Most catheters used in EVD (such as Integra®, Medtronic®, and Codman®) measure longer than 30 cm and there is sufficient space to include color bands, as outlined in our approach, on clinical catheters. To further mitigate occlusion-related concerns around color bands, one could explore adding additional redundant color bands. Last but not least, attention needs to be paid to the clinical safety of catheter modification. Technologies such as VisiMark®⁴ could be used to create medical-grade markings to serve as the color bands. Alternatively, the catheter could be constructed with medical-grade silicone of various colors and go through standard sterilization. Slight changes would need to be made to the color band detection process.

7 CONCLUSION

We present an augmented reality surgical visualization and tracking system that can assist surgeons in EVD catheter placement. Compared to existing similarly-purposed systems, our system does not require changing the shape or weight of the medical instruments. Our main technical contributions include 1) a low-latency, high-performance way to track catheters and other 5DOF thin cylindrical objects, and 2) an image processing algorithm to extract tracking color segment endpoints in an image. Tests show that our tracking method achieves a 0.58 mm accuracy on a 2D plane and an accuracy of 0.85 mm in 3D space. Processing for each frame takes 22.60 ms on a moderately powerful computer. Both the accuracy and speed can be further improved with higher-quality cameras and parallel implementation. We have tested our system in a realistic surgical environment with a cadaveric head. Our color marker and tracking technique can be applied to other medical procedures where the precise location of a very thin medical instrument is needed, such as needle-guided biopsies and minimally invasive surgeries.

⁴<http://www.surfacegroup.com/coatings/visi-mark/>

ACKNOWLEDGMENTS

We sincerely appreciate the anonymous reviewers for their insightful and exceptionally thorough reviews that have greatly helped us in improving this paper. We would also like to thank Barbara Brawn-Cinani for her constructive advice and comments that were vital to refining our presentation and Jonathan Heagerty for his help with designing and fabricating the necessary tools for testing our system. This work has been supported in part by the NSF Grants 18-23321, 16-32976, 15-64212, 14-29404, and the State of Maryland MPower initiative. Any opinions, findings, conclusions, or recommendations expressed in this article are those of the authors and do not necessarily reflect the views of the research sponsors.

REFERENCES

- Yuichiro Abe, Shigenobu Sato, Koji Kato, Takahiko Hyakumachi, Yasushi Yanagibashi, Manabu Ito, and Kuniyoshi Abumi. 2013. A novel 3D guidance system using augmented reality for percutaneous vertebroplasty. *Journal of Neurosurgery: Spine* 19, 4 (2013), 492–501.
- Kamyar Abhari, John S. H. Baxter, Elvis C. S. Chen, Ali R. Khan, Terry M. Peters, Sandrine de Ribaupierre, and Roy Eagleson. 2014. Training for planning tumour resection: augmented reality and human factors. *IEEE Transactions on Biomedical Engineering* 62, 6 (2014), 1466–1477.
- Marc-André Ameller, Bill Triggs, and Long Quan. 2000. Camera Pose Revisited-New Linear Algorithms. (2000).
- Ehsan Azimi, Camilo Molina, Alexander Chang, Judy Huang, Chien-Ming Huang, and Peter Kazanides. 2018. Interactive Training and Operation Ecosystem for Surgical Tasks in Mixed Reality. In *OR 2.0 Context-Aware Operating Theaters, Computer Assisted Robotic Endoscopy, Clinical Image-Based Procedures, and Skin Image Analysis*. Springer, 20–29.
- P. Pat Banerjee, Cristian J. Luciano, G. Michael Lemole Jr, Fady T. Charbel, and Michael Y. Oh. 2007. Accuracy of ventriculostomy catheter placement using a head-and hand-tracked high-resolution virtual reality simulator with haptic feedback. *Journal of Neurosurgery* 107, 3 (2007), 515–521.
- Ehsan Basafa, Pezhman Foroughi, Martin Hossbach, Jasmine Bhanushali, and Philipp Stolka. 2017. Visual tracking for multi-modality computer-assisted image guidance. In *Medical Imaging 2017: Image-Guided Procedures, Robotic Interventions, and Modeling*, Vol. 10135. International Society for Optics and Photonics, 101352S.
- Olivier Cros, Morten Volden, Jens Jørgen Flaaris, Lars Chebørlov Brix, Christian Fischer Pedersen, Kim Vang Hansen, Ole Vilhelm Larsen, Lasse Riis Østergaard, and Jens Haase. 2002. Simulating the puncture of the human ventricle. In *10th Annual Medicine Meets Virtual Reality Conference*.
- Andrew Benjamin Cutler, Shervin Rahimpour, Yameng Liu, Nandan Lad, Regis Kopper, and Patrick Codd. 2017. Development of Augmented Reality-Based Neuro-Navigation System for use in External Ventricular Drain Placement. In *Journal of Neurosurgery*, Vol. 126. A1438–A1438. <https://youtu.be/qqykWW9f41Q>
- Ruofei Du, Ming Chuang, Wayne Chang, Hugues Hoppe, and Amitabh Varshney. 2019. Montage4D: Real-time Seamless Fusion and Stylization of Multiview Video Textures. *Journal of Computer Graphics Techniques* 8, 1 (17 January 2019), 1–34. <https://doi.org/10.1145/3190834.3190843>
- Philip J. Edwards, Derek L. G. Hill, David J. Hawkes, R. Spink, Alan C. F. Colchester, A. Strong, and M. Gleeson. 1995. Neurosurgical guidance using the stereo microscope. In *Computer Vision, Virtual Reality and Robotics in Medicine*. Springer, 555–564.
- Philip J. Edwards, Laura G. Johnson, David J. Hawkes, Michael R. Fenlon, Anthony J. Strong, and Michael J. Gleeson. 2004. Clinical experience and perception in stereo augmented reality surgical navigation. In *International Workshop on Medical Imaging and Virtual Reality*. Springer, 369–376.
- P. J. Edwards, A. P. King, C. R. Maurer, D. A. De Cunha, D. J. Hawkes, D. L. G. Hill, R. P. Gaston, M. R. Fenlon, A. Jusczyck, A. J. Strong, C. L. Chandler, and M. J. Gleeson. 2000. Design and evaluation of a system for microscope-assisted guided interventions (MAGI). *IEEE Transactions on Medical Imaging* 19, 11 (2000), 1082–1093.
- Zhencheng Fan, Guowen Chen, Junchen Wang, and Hongen Liao. 2017. Spatial Position Measurement System for Surgical Navigation using 3-D Image Marker-based Tracking Tools with Compact Volume. *IEEE Transactions on Biomedical Engineering* 65, 2 (2017), 378–389.
- Taylor Frantz, Bart Jansen, Johnny Duerinck, and Jef Vandemeulebroucke. 2018. Augmenting Microsoft’s HoloLens with vuforia tracking for neuronavigation. *Healthcare technology letters* 5, 5 (2018), 221–225.
- Herbert I. Fried, Barnett R. Nathan, A Shaun Rowe, Joseph M. Zabramski, Norberto Andaluz, Adarsh Bhimraj, Mary McKenna Guanci, David B. Seder, and Jeffrey M. Singh. 2016. The insertion and management of external ventricular drains: an evidence-based consensus statement. *Neurocritical care* 24, 1 (2016), 61–81.
- Xiao-Shan Gao, Xiao-Rong Hou, Jianliang Tang, and Hang-Fei Cheng. 2003. Complete solution classification for the perspective-three-point problem. *IEEE transactions on pattern analysis and machine intelligence* 25, 8 (2003), 930–943.

- Daipayan Guha, Naif M Alotaibi, Nhu Nguyen, Shaurya Gupta, Christopher McFaul, and Victor X. D. Yang. 2017. Augmented reality in neurosurgery: a review of current concepts and emerging applications. *Canadian Journal of Neurological Sciences* 44, 3 (2017), 235–245.
- David R. Huyette, Benjamin J. Turnbow, Christian Kaufman, Dale F. Vaslow, Benjamin B. Whiting, and Michael Y. Oh. 2008. Accuracy of the freehand pass technique for ventriculostomy catheter placement: retrospective assessment using computed tomography scans. *Journal of Neurosurgery* 108, 1 (2008), 88–91.
- D Inoue, B Cho, M Mori, Y Kikkawa, T Amano, A Nakamizo, K Yoshimoto, M Mizoguchi, M Tomikawa, J Hong, M. Hashizume, and T. Sasaki. 2013. Preliminary study on the clinical application of augmented reality neuronavigation. *Journal of Neurological Surgery Part A: Central European Neurosurgery* 74, 02 (2013), 071–076.
- Calvin R. Maurer Jr., Frank Sauer, Bo Hu, Benedicte Bascle, Bernhard Geiger, Fabian Wenzel, Filippo Recchi, Torsten Rohlfing, Christopher R. Brown, Robert J. Bakos, Robert J. Maciunas, and Ali R. Bani-Hashemi. 2001. Augmented reality visualization of brain structures with stereo and kinetic depth cues: System description and initial evaluation with head phantom. *Medical Imaging 2001* (2001), 445–456.
- Udaya K. Kakarla, Louis J. Kim, Steven W. Chang, Nicholas Theodore, and Robert F. Spetzler. 2008. Safety and accuracy of bedside external ventricular drain placement. *Operative Neurosurgery* 63, suppl_1 (2008), ONS162–ONS167.
- Marta Kersten-Oertel, Pierre Jannin, and D. Louis Collins. 2013. The state of the art of visualization in mixed reality image guided surgery. *Computerized Medical Imaging and Graphics* 37, 2 (2013), 98–112.
- Ralf A. Kockro, Yeo Tseng Tsai, Ivan Ng, Peter Hwang, Chuangui Zhu, Kusuma Agusanto, Liang Xiao Hong, and Luis Serra. 2009. Dex-ray: augmented reality neurosurgical navigation with a handheld video probe. *Neurosurgery* 65, 4 (2009), 795–808.
- G. Krombach, A. Ganser, Ch Fricke, V. Rohde, M. Reinges, J. Gilsbach, and U. Spetzger. 2000. Virtual placement of frontal ventricular catheters using frameless neuronavigation: an “unbloody training” for young neurosurgeons. *Minimally Invasive Neurosurgery* 43, 04 (2000), 171–175.
- Timur Kuzhagaliyev, Neil T. Clancy, Mirek Janatka, Kevin Tchaka, Francisco Vasconcelos, Matthew J. Clarkson, Kurinchi Gurusamy, David J. Hawkes, Brian Davidson, and Danail Stoyanov. 2018. Augmented reality needle ablation guidance tool for irreversible electroporation in the pancreas. In *Medical Imaging 2018: Image-Guided Procedures, Robotic Interventions, and Modeling*, Vol. 10576. International Society for Optics and Photonics, 1057613.
- G. Michael Lemole Jr, P. Pat Banerjee, Cristian Luciano, Sergey Neckrysh, and Fady T. Charbel. 2007. Virtual reality in neurosurgical education: part-task ventriculostomy simulation with dynamic visual and haptic feedback. *Neurosurgery* 61, 1 (2007), 142–149.
- Ye Li, Xiaolei Chen, Ning Wang, Wenyao Zhang, Dawei Li, Lei Zhang, Xin Qu, Weitao Cheng, Yueqiao Xu, Wenjin Chen, and Qiumei Yang. 2018. A wearable mixed-reality holographic computer for guiding external ventricular drain insertion at the bedside. *Journal of Neurosurgery* 1, aop (2018), 1–8.
- M. A. Lin, A. F. Siu, J. H. Bae, M. R. Cutkosky, and B. L. Daniel. 2018. HoloNeedle: Augmented Reality Guidance System for Needle Placement Investigating the Advantages of Three-Dimensional Needle Shape Reconstruction. *IEEE Robotics and Automation Letters* 3, 4 (Oct 2018), 4156–4162. <https://doi.org/10.1109/LRA.2018.2863381>
- Eduardo E. Lovo, Juan C. Quintana, Manuel C. Puebla, Gonzalo Torrealba, José L. Santos, Isidro H. Lira, and Patricio Tagle. 2007. A novel, inexpensive method of image coregistration for applications in image-guided surgery using augmented reality. *Operative Neurosurgery* 60, suppl_4 (2007), ONS–366.
- David Low, Cheng Kiang Lee, Lee Lian Tay Dip, Wai Hoe Ng, Beng Ti Ang, and Ivan Ng. 2010. Augmented reality neurosurgical planning and navigation for surgical excision of parasagittal, falicine and convexity meningiomas. *British Journal of Neurosurgery* 24, 1 (2010), 69–74.
- Cristian Luciano, Pat Banerjee, G. Michael Lemole, and Fady Charbel. 2005. Second generation haptic ventriculostomy simulator using the ImmersiveTouch™ system. *Studies in health technology and informatics* 119 (2005), 343.
- Eric Marchand, Hideaki Uchiyama, and Fabien Spindler. 2016. Pose estimation for augmented reality: a hands-on survey. *IEEE transactions on visualization and computer graphics* 22, 12 (2016), 2633–2651.
- Yoshitaka Masutani, Takeyoshi Dohi, Fumitaka Yamane, Hiroshi Iseki, and Kintomo Takakura. 1998. Augmented reality visualization system for intravascular neurosurgery. *Computer aided surgery* 3, 5 (1998), 239–247.
- Xiaoxu Meng, Ruofei Du, Matthias Zwicker, and Amitabh Varshney. 2018. Kernel Foveated Rendering. *Proceedings of the ACM on Computer Graphics and Interactive Techniques (I3D)* 1, 5 (15 - 18 May 2018), 1–20. <https://doi.org/10.1145/3203199>
- Antonio Meola, Fabrizio Cutolo, Marina Carbone, Federico Cagnazzo, Mauro Ferrari, and Vincenzo Ferrari. 2016. Augmented reality in neurosurgery: a systematic review. *Neurosurgical review* (2016), 1–12.
- Mohammad Najafi, Purang Abolmaesumi, and Robert Rohling. 2015. Single-camera closed-form real-time needle tracking for ultrasound-guided needle insertion. *Ultrasound in medicine & biology* 41, 10 (2015), 2663–2676.
- Mohammad Najafi and Robert Rohling. 2011. Single camera closed-form real-time needle trajectory tracking for ultrasound. In *Medical Imaging 2011: Visualization, Image-Guided Procedures, and Modeling*, Vol. 7964. International Society for Optics and Photonics, 79641F.

- Diederick C Niehorster, Li Li, and Markus Lappe. 2017. The Accuracy and Precision of Position and Orientation Tracking in the HTC Vive Virtual Reality System for Scientific Research. *i-Perception* 8, 3 (2017), 177–205.
- Shaun T. O’Leary, Max K. Kole, Devon A. Hoover, Steven E. Hysell, Ajith Thomas, and Christopher I. Shaffrey. 2000. Efficacy of the Ghajar Guide revisited: a prospective study. *Journal of neurosurgery* 92, 5 (2000), 801–803.
- Nicholas I. Phillips and Nigel W. John. 2000. Web-based surgical simulation for ventricular catheterization. *Neurosurgery* 46, 4 (2000), 933–937.
- Long Quan and Zhongdan Lan. 1999. Linear n-point camera pose determination. *IEEE Transactions on pattern analysis and machine intelligence* 21, 8 (1999), 774–780.
- Faith C. Robertson, Muhammad M. Abd-El-Barr, Srinivasan Mukundan, and William B. Gormley. 2017. Ventriculostomy-associated hemorrhage: a risk assessment by radiographic simulation. *Journal of neurosurgery* 127, 3 (2017), 532–536.
- Frank Sauer, Ali Khamene, Benedicte Bascle, and Gregory J. Rubino. 2001. A head-mounted display system for augmented reality image guidance: Towards clinical evaluation for imri-guided neurosurgery. In *Proceedings of the 4th International Conference on Medical Image Computing and Computer-Assisted Intervention*. Springer-Verlag, 707–716.
- Clemens M. Schirmer, J. Bradley Elder, Ben Roitberg, and Darlene A. Lobel. 2013. Virtual reality-based simulation training for ventriculostomy: an evidence-based approach. *Neurosurgery* 73, suppl_1 (2013), S66–S73.
- M. Scholz, W. Konen, S. Tombrock, B. Fricke, L. Adams, M. Von Duering, A. Hentsch, L. Heuser, and A. G. Harders. 1998. Development of an endoscopic navigation system based on digital image processing. *Computer Aided Surgery* 3, 3 (1998), 134–143.
- Ramin Shahidi, Bai Wang, Marc Epitoux, Robert Grzeszczuk, and John Adler. 1998. Volumetric image guidance via a stereotactic endoscope. *Medical Image Computing and Computer-Assisted Intervention* (1998), 241–252.
- Visish M. Srinivasan, Brent R. O’Neill, Diana Jho, Donald M. Whiting, and Michael Y. Oh. 2014. The history of external ventricular drainage: Historical vignette. *Journal of neurosurgery* 120, 1 (2014), 228–236.
- Philipp J. Stolka, Pezhman Foroughi, Matthew Rendina, Clifford R. Weiss, Gregory D. Hager, and Emad M. Boctor. 2014. Needle Guidance Using Handheld Stereo Vision and Projection for Ultrasound-Based Interventions. In *Medical Image Computing and Computer-Assisted Intervention – MICCAI 2014*, Polina Golland, Nobuhiko Hata, Christian Barillot, Joachim Hornegger, and Robert Howe (Eds.). Springer International Publishing, Cham, 684–691.
- Xuetong Sun and Amitabh Varshney. 2018. Investigating Perception Time in the Far Peripheral Vision for Virtual and Augmented Reality. In *Proceedings of the 15th ACM Symposium on Applied Perception (SAP ’18)*. ACM, New York, NY, USA, Article 13, 8 pages. <https://doi.org/10.1145/3225153.3225160>
- Bruce L. Tai, Deborah Rooney, Francesca Stephenson, Peng-Siang Liao, Oren Sagher, Albert J. Shih, and Luis E. Savastano. 2015. Development of a 3D-printed external ventricular drain placement simulator. *Journal of neurosurgery* 123, 4 (2015), 1070–1076.
- Peter Y. M. Woo, Ben C. F. Ng, Jacob X. Xiao, Daniel Wong, Andrew Seto, Sandy Lam, Carmen Yim, Hong-Yip Lo, Yin-Chung Po, Larry Y. W. Wong, Michael W. Y. Lee, Kwong-Yui Yam, Jenny K. S. Pu, Kwong-Yau Chan, and Wai-Sang Poon. 2019. The importance of aspirin, catheterization accuracy, and catheter design in external ventricular drainage-related hemorrhage: a multicenter study of 1002 procedures. *Acta Neurochirurgica* (2019), 1–10.
- Rachel Yudkowsky, Cristian Luciano, Pat Banerjee, Alan Schwartz, Ali Alaraj, G. Michael Lemole Jr, Fady Charbel, Kelly Smith, Silvio Rizzi, Richard Byrne, Bernard Bendok, and David Frim. 2013. Practice on an augmented reality/haptic simulator and library of virtual brains improves residents’ ability to perform a ventriculostomy. *Simulation in Healthcare* 8, 1 (2013), 25–31.